



Zen-X DCiS

DC Wireless intraoral sensor



www.my-ray.com





BU Medical Equipment

Plant - Via Bicocca, 14/c - 40026 Imola - Bo (Italy) tel. +39 0542 653441 - fax +39 0542 653555

Headquarters - Cefla s.c. Via Selice Provinciale, 23/a - 40026 Imola - Bo (Italy) tel. +39 0542 653111 - fax +39 0542 653344

Cefla Medical North America

6125 Harris Technology Blvd. - Charlotte, NC 28269 - Ph: 704 598 0020 - www.ceflamedicalna.com - info@cefladental.com

As simple as freedom!

The first intraoral sensor with Wire Free system and DC (Direct Conversion), for accurate X-ray imaging in just a few steps. Cordless for maximum usability. Compact and ergonomic for patient comfort.

Wire Free. To be free.



IP67 certified for protection against liquids and dust.

ALL IN ONE Docking station for housing and charging the sensor when not in use.











WIRE FREE

COMPACT

Less stress for the patient with rounded edges.

Minimum thickness thanks to Direct Conversion (DC) technology which streamlines the number of internal components. Extremely slim rechargeable lithium

battery housing hub.

Antenna for data reception in Wireless mode: minimum consumption, maximum image yield.

WHEREVER YOU WANT

Place your docking station on a work surface, on your desk or on the wall using the special fixing kit. Status LED always visible. Simple and always accessible USB connection.

Efficient and patient-friendly.

Enhance your workflow and patient experience with Zen-X DCiS. The right tool to get the most out of your time.

Experience the convenience of our Wire Free system: no cables to hinder movements; no stress for the patient thanks to the sensor low thickness and rounded corners; accessories to facilitate positioning while minimising discomfort for the patient.

Since the cable is the part most exposed to wear, the Wire Free system also guarantees a longer sensor life.

Zen-X DCiS, integrating direct conversion technology, has no internal easily breakable components and is therefore more resistant to falls and impacts.

Simply the best.

- Compact and minimally invasive
- Cordless
- Easy positioning





DESIGNED TO LAST

Stronger outer shell and internal components for increased impact and compression resistance and a longer life. No fragile components such as the scintillator which is required in sensors that do not integrate DC technology.



Non-invasive sensor thanks to its extremely low thickness and smooth lines without edges. Zen-X DCiS puts patient health and care first.



POSITIONING

Alignment system created specifically for Zen-X DCiS that does not add extra bulk to the sensor profile and guarantees superior patient comfort.

Easy to position, it allows the X-ray unit to be brought closer to the patient face exposing only the required areas - thanks to a special alignment ring and positioners designed to adapt perfectly to specific diagnostic needs.

The ultimate 2D imaging.


First wireless direct conversion sensor. Zen-X DCiS incorporates all the best high-tech imaging technologies.

Zen-X DCiS integrates direct conversion technology, which does not require the conversion of X-rays into visible light. Fewer steps, fewer components, smaller footprint and above all - perfect image quality. Once scanning is complete, iRYS will take care of everything.

MyRay's native software features advanced filters to further enhance the image or emphasize details.

Less is more.

- Fewer required steps More sharpness
- Better contrast
- Minimal bulk
- Long life

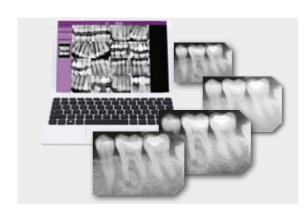

MultiMAGE

This original MyRay function is designed to meet the real needs of dentists like you.

By using proprietary PiE (Powerful image Enhancer) algorithms optimised for the Zen-X DCiS sensor, this function lets dentists simultaneously capture, display and share a set of up to 5 images. Each image is the result of a different type of improvement designed to highlight various anatomical details with different levels of sharpness and contrast, ensuring dentists can diagnose better.




SOFT TISSUE PRESERVING



darkening unaltered to highlight soft tissues.

High contrast: enhances the contrast, if the image is low in contrast due to anatomical reasons or X-ray parameters.






Caries revealing: improves the contrast level of bitewing images allowing easier identification of interproximal caries.

Default: balances noise, contrast and sharpness.





CARIES REVEALING

IN-DEPTH DETAIL

The best of 2D X-ray imaging: Zen-X DCiS direct conversion sensor produces sharper images with better contrast than a conventional sensor.











THE BENEFITS OF DIRECT CONVERSION

With a standard sensor X-rays have to be converted into visible light, using a scintillator, because the sensor reacts to light like a photographic film. Zen-X DCiS, on the other hand, is a direct conversion sensor: it receives and processes X-rays directly. Fewer steps mean a lower risk of diagnostic information loss, sharper and well-contrasted images, even at low doses.

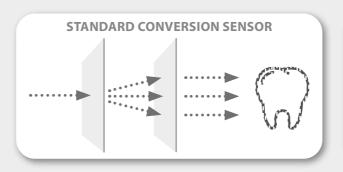

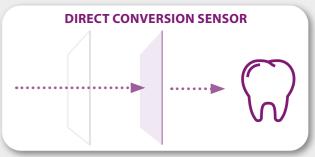

Your best workflow solution.

Choose the configuration that best suits your needs. The sensor adapts to your work, not the other way around.

Zen-X DCiS streamlines your workflow and integrates seamlessly into your clinic. Through Wireless technology, the sensor interacts with the docking station wirelessly and with minimum power consumption with no impact on quality.

In just a few seconds the image is available on the monitor to be shared with the patient and colleagues.


With iRYS you can browse through images, calibrate them or use pre-settable filters. The software allows pairing with the dentition chart and has predefined layouts to quickly store and view the X-rays.


A preferred combination of sensors and docking station can also be chosen. Zen-X DCiS is made to look like you!

It fits!

- Images available immediately
- Several possible configurations
- Energy saving



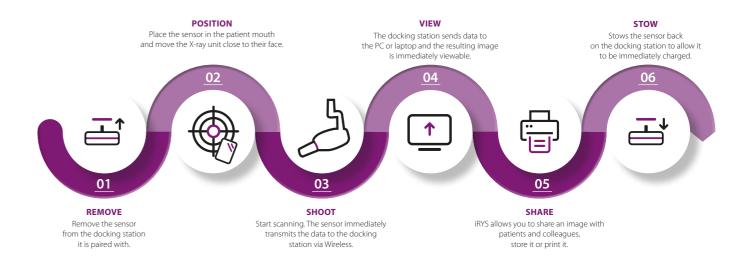




WORKFLOW A

1 to 1 pairing.


Each sensor interacts with its own docking station. Simultaneous data transmission is also possible.

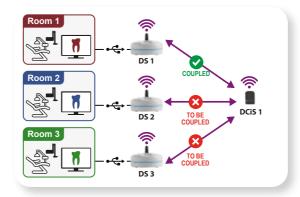

WORKFLOW B

1 to many pairing.

A single sensor interacts with multiple docking stations. The sensor can interact with only one docking station at a time.



WORKFLOW C

Many to 1 pairing.

Several sensors interact with a single docking station. Transmission can occur from only one sensor at a time.

Zen-X DCiS • DC Wireless. 12

Optional accessories.

Add the alignment system designed for Zen-X DCiS. Choose where to keep the docking station. Optimized ergonomics and maximum user-friendliness.

Alignment system that facilitates positioning. No extra bulk for the sensor profile which is therefore minimally invasive in the patient's mouth for superior comfort.

The system allows the X-ray unit to be brought closer to the patient's face, focussing the X-ray emission only on the area to be examined.

A special kit allows you to install the docking station on the wall, freeing up workspace.

It's that easy!

- Minimally invasive in the mouth
- Easy positioning
- Optimal alignment
- Wall fixing of the docking station







Technical specifications.

Sensor size 2 Sensor footprint 43.4 mm (height) x 29.5 mm (width) Sensor thickness 5.2 mm (9.2 mm considering the battery housing hub) Active area 35.1 mm x 24.7 mm Docking station 100 mm (diameter) x 6.2 mm (height) USB lead length 2 m (supplied to connect docking station to PC/laptop) WAGE ACQUISITION Pixel matrix 1350 x 950 (1,282,500 pixel) Detector Single-crystal direct-conversion silicon / CMOS MTF (Modulation Transfer Function) 2 70% @ 5 [p/mm, > 40% @ 10 [p/mm Exposure parameters 0.1-0.5 x 6,607 0.4% / 68 mm, 20 cm (81 cone Wireless image transmission time SENSOR TECHNICAL SPECIFICATIONS Internal battery Rechargeable lithium ion (capacity 19 mAH) Degree of protection IP 67 (Guaranteed against liquid or dust infiltration) Integrated RAM memory 4 MB (maximum 1 preservable image) Wireless operating distance Compatibility with X-ray generators Compatibility with X-ray generators Complete recharge time 3.5 h fallows acquisition of 140° consecutive images, with a 40 s pause between two examinations) Minimum advisable recharge time 15 minutes (allows acquisition of 140° consecutive images, with a 40 s pause between two examinations) Integrated protocols DicOM nodes Wireless Management software (for PC) IRYS (complies with ISDP*100032020 as per EN ISO/EC 17065:2012 certificate number 2019003109-2) Supported operating systems Minimum Advisable recharge time (First, Storage Commitment, SR document; WorkList, MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft* Windows* 10 Pro 6 A bit in Vindows* 11 Pro 6 4 bit vindows* 11 Pro		DIMENSIONS	
Sensor footprint Sensor thickness Sensor		DIMENSIONS	
Sensor thickness 5.2 mm (9.2 mm considering the battery housing hub) Active area 3.5.1 mm x 24.7 mm 100 mm (diameter) x 62 mm (height) USB lead length 2 m (supplied to connect docking station to PC/laptop) IMAGE ACQUISITION			
Active area 35.1 mm x 24.7 mm Docking station 100 mm (dameter) x 62 mm (height) 100 Blead length 2 m (supplied to connect docking station to PC/laptop) IMAGE ACQUISITION 1350 x 950 (1,282,500 pixel) Pixel matrix 1350 x 950 (1,282,500 pixel) Single-crystal direct-conversion silicon / CMOS MTF (Modulation Transfer Function) > 70% @ 5 lp/mm, > 40% @ 10 lp/mm Exposure parameters 0.1-0.5 x, 60-70 kV, 6/8 mA, 20 cm (87) cone Exersion single transmission item SENSOR TECHNICAL SPECIFICATIONS Internal battery Rechargeable lithium ion (capacity 19 mAH) Poegree of protection P67 (Guaranteed against liquid or dust infiltration) Integrated RAM memory 4 MB (maximum 1 preservable image) Wireless United Statistics Up to 2.5 m from docking station Wireless Organizating distance Up to 2.5 m from docking station Up to 2.5 m from docking station Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV. Portable: 2-10 mA and 60-70 kV. Complete recharge time 3.5 h (allows acquisition of 140° consecutive images, with a 40 s pause between two examinations) Infinity and software (for PC) Icapture with dedicated filters for third party software (for PC) Icapture with dedicated filters for third party software (for PC) ICapture with dedicated filters for third party software (for PC) ICAPTURE (Expolication of 140° consecutive images, with a 40 s pause between two examinations) DICOM 3.0, TWAIN, VDDS INEGENORAL (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft* Windows* 10 Pro 64 bit - Windows* 11 Pro 64 bit Print (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft* Windows* 10 Pro 64 bit - Windows* 11 Pro 64 bit Print (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft* Windows* 10 Pro 64 bit - Windows* 11 Pro 64 bit Print (Print; Storage Commi			
Docking station 100 mm (diameter) x 62 mm (height) 2 m (supplied to connect docking station to PC/laptop) MAGE ACQUISITION			
USB lead length 2 m (supplied to connect docking station to PC/laptop) IMAGE ACQUISITION 1350 x 950 (1282,500 pixel) Detector Single-crystal direct-conversion silicon / CMOS MTF (Modulation Transfer Function) > 70% ⊚ 5 [p/mm, ≥ 40% ⊚ 10 [p/mm Exposure parameters 0.1-0.5 x, 60~70 kV, 6/8 mA, 20 cm (87) cone Wireless image transmission time Less than 10 s under optimal working conditions SENSOR TECHNICAL SPECIFICATIONS Integrated RAM memory Rechargeable lithium ion (capacity 19 mAH) Pegree of protection Integrated RAM memory 4 MB (maximum 1 preservable image) Wireless Up to 2.5 m from docking station Compatibility with X-ray generators Complete recharge time 3.5 h (allows acquisition of 140° consecutive images, with a 40 s pause between two examinations) Minimum advisable recharge time 3.5 h (allows acquisition of 19° consecutive images, with a 40 s pause between two examinations) **SOFTWARE** Acquisition software (for PC) Image management software (for PC) Ima	Active area		
IMAGE ACQUISITION 1350 x 950 (1,282,500 pixel)	Docking station	100 mm (diameter) x 62 mm (height)	
Pixel matrix 1350 x 950 (1,282,500 pixel) Detector Single-crystal direct-conversion silicon / CMOS MTF (Modulation Transfer Function) ≥ 70% @ 5 lp/mm, ≥ 40% @ 10 lp/mm Exposure parameters 0.1-0.5 s, 60-70 kV, 6/8 mA, 20 cm (8°) cone Wireless image transmission time Less than 10 s under optimal working conditions SENSOR TECHNICAL SPECIFICATIONS Internal battery Rechargeable lithium ion (capacity 19 mAH) Degree of protection IP 67 (Guaranteed against liquid or dust infiltration) Integrated RAM memory 4 MB (maximum 1 preservable image) Ilmage transmission technology Wireless Wireless operating distance Up to 2.5 m from docking station Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV. Portable: 2-10 mA and 60-70 kV. Complete recharge time 3.5 h (allows acquisition of 140° consecutive images, with a 40 s pause between two examinations) Minimum advisable recharge time 3.5 h (allows acquisition of 140° consecutive images, with a 40 s pause between two examinations) SOFTWARE Acquisition software (for PC) iCapture with dedicated filters for third party software Image management software (for PC) iCapture with dedicated filters for third party software iRYS (complies with iSDP*10003/200 as per EN ISO/IEC17065:2012 certificate number 2019003109-2) Supported protocols DICOM 3.0, TWAIN, VDDS DICOM 3.0, TWAI	USB lead length		
Detector Single-crystal direct-conversion silicon / CMOS MTF (Modulation Transfer Function) > 70% & 5 1p/mm, > 40% & 91 1p/mm Exposure parameters 0.1-0.5 s, 60-70 kl, 6% mA, 20 cm (8") cone Wireless image transmission time Less than 10 s under optimal working conditions **SENSOR TECHNICAL SPECIFICATIONS** Internal battery Rechargeable lithium ion (capacity 19 mAH) Degree of protection IP 67 (Guaranteed against liquid or dust infiltration) Integrated RAM memory 4 MB (maximum 1 preservable image) Image transmission technology Wireless Wireless operating distance Up to 2.5 m from docking station Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kl/. Portable: 2-10 mA and 60-70 kl/. Complete recharge time 3.5 h (allows acquisition of 140" consecutive images, with a 40 s pause between two examinations) Minimum advisable recharge time 15 minutes (allows acquisition of 19" consecutive images, with a 40 s pause between two examinations) **SOFTWARE** Acquisition software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) ICAPTURE with ISDP*10003:2020 as per EN ISO/IEC17065:2012 certificate number 2019003109-2) **SUpported protocols DICOM 3.0, TWAIN, VDDS DICOM nodes IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) **MINIMUM SYSTEM REQUISITES** Supported operating systems Microsoft** Windows** 10 Pro 64 bit - Windows** 11 Pro 64 bit Processor 6th generation Intel 15 or equivalent Hard disk Intel Core 13, 10th generation (or higher) **ARM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD **COMMUNICATION INTERFACES** **Docking station connection port USB-A** Power supply +5V ± 10%*			
MTF (Modulation Transfer Function) > 70% @ 5 lp/mm, > 40% @ 10 lp/mm Exposure parameters 0.1-0.5 s, 60-70 kV, 6/8 mA, 20 cm (8°) cone Wireless image transmission time SENSOR TECHNICAL SPECIFICATIONS Internal battery Rechargeable lithium ion (capacity 19 mAH) Degree of protection IP 67 (Guaranteed against liquid or dust infiltration) Integrated RAM memory Integrated RAM memory Image transmission technology Wireless Wireless Wireless operating distance Up to 2.5 m from docking station Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV. Portable: 2-10 mA and 60-70 kV. Complete recharge time 3.5 h (allows acquisition of 140° consecutive images, with a 40 s pause between two examinations) SOFTWARE Acquisition software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Image management software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Icapture with dedicated filters for third party software Image management softwar	Pixel matrix		
Exposure parameters 0.1-0.5 s, 60-70 kV, 6/8 mA, 20 cm (8") cone Wireless image transmission time Less than 10 s under optimal working conditions SENSOR TECHNICAL SPECIFICATIONS Internal battery Rechargeable lithium ion (capacity 19 mAH) Degree of protection IP 67 (Guaranteed against liquid or dust infiltration) Integrated RAM memory 4 MB (maximum 1 preservable image) Image transmission technology Wireless Wireless Wireless operating distance Up to 2.5 m from docking station Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV. Portable: 2-10 mA and 60-70 kV. Complete recharge time 3.5 h (allows acquisition of 140" consecutive images, with a 40 s pause between two examinations) If minutes (allows acquisition of 19" consecutive images, with a 40 s pause between two examinations) SOFTWARE Acquisition software (for PC) iCapture with dedicated filters for third party software Image management software (for PC) iRYS (complies with ISDP®10003:2020 as per EN ISO/IEC17065:2012 certificate number 2019003109-2) Supported protocols DICOM 3.0, TWAIN, VDDS DICOM nodes IHE compliant (Print, Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft® Windows® 10 Pro 64 bit - Windows® 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/Japtop connection port USB-C PC/Japtop connection port USB-C PC/Japtop connection port USB-C PC/Japtop connection port USB-C	Detector	Single-crystal direct-conversion silicon / CMOS	
Wireless image transmission time Less than 10 s under optimal working conditions SENSOR TECHNICAL SPECIFICATIONS Internal battery Rechargeable lithium ion (capacity 19 mAH) Degree of protection IP 67 (Guaranteed against liquid or dust infiltration) Integrated RAM memory 4 MB (maximum 1 preservable image) Wireless Wireless Wireless Wireless operating distance Up to 2.5 m from docking station Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV. Portable: 2-10 mA and 60-70 kV. Complete recharge time 3.5 h (allows acquisition of 140* consecutive images, with a 40 s pause between two examinations) In minutes (allows acquisition of 19* consecutive images, with a 40 s pause between two examinations) SOFTWARE Acquisition software (for PC) iCapture with dedicated filters for third party software Image management software (for PC) iRYS (complies with ISDP*10003:2020 as per EN ISO/IEC17065:2012 certificate number 2019003109-2) Supported protocols DICOM 3.0, TWAIN, VDDS IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft* Windows* 10 Pro 64 bit - Windows* 11 Pro 64 bit Processor 6th generation Intel 15 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/Japtop connection port USB-C	MTF (Modulation Transfer Function)	> 70% @ 5 lp/mm, > 40% @10 lp/mm	
Internal battery Rechargeable lithium ion (capacity 19 mAH) Degree of protection IP 67 (Guaranteed against liquid or dust infiltration) Integrated RAM memory 4 MB (maximum 1 preservable image) Image transmission technology Wireless Wireless Wireless operating distance Up to 2.5 m from docking station Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV. Portable: 2-10 mA and 60-70 kV. Complete recharge time 3.5 h (allows acquisition of 140° consecutive images, with a 40 s pause between two examinations) Minimum advisable recharge time 15 minutes (allows acquisition of 19° consecutive images, with a 40 s pause between two examinations) SOFTWARE Acquisition software (for PC) iCapture with dedicated filters for third party software Image management software (for PC) iRYS (complies with ISDP°10003:2020 as per EN ISO/IEC17065:2012 certificate number 2019003109-2) Supported protocols DICOM 3.0, TWAIN, VDDS IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft* Windows* 10 Pro 64 bit - Windows* 11 Pro 64 bit Processor 6th generation Intel 15 or equivalent Intel Core 13, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-A Power supply +5V ± 10%	Exposure parameters	0.1-0.5 s, 60-70 kV, 6/8 mA, 20 cm (8") cone	
Internal battery Degree of protection IP 67 (Guaranteed against liquid or dust infiltration) Integrated RAM memory 4 MB (maximum 1 preservable image) Image transmission technology Wireless Wireless operating distance Up to 2.5 m from docking station Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV, Portable: 2-10 mA and 60-70 kV. Complete recharge time 3.5 h (allows acquisition of 140* consecutive images, with a 40 s pause between two examinations) In minum advisable recharge time SOFTWARE Acquisition software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) ICAPTURE DICOM 3.0, TWAIN, VDDS IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Microsoft* Windows* 10 Pro 64 bit - Windows* 11 Pro 64 bit Processor Alard disk Intel Core i3, 10th generation (nr higher) RAM 4 GB (8 GB or superior recommended) Graphics card JD Video Card 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display Docking station connection port USB-C PC/Japtop connection port USB-A Power supply +5V ± 1096	Wireless image transmission time	Less than 10 s under optimal working conditions	
Degree of protection IP 67 (Guaranteed against liquid or dust infiltration) Integrated RAM memory 4 MB (maximum 1 preservable image) Image transmission technology Wireless Wireless operating distance Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV. Portable: 2-10 mA and 60-70 kV. Complete recharge time 3.5 h (allows acquisition of 140* consecutive images, with a 40 s pause between two examinations) Minimum advisable recharge time 15 minutes (allows acquisition of 19* consecutive images, with a 40 s pause between two examinations) SOFTWARE Acquisition software (for PC) icapture with dedicated filters for third party software Image management software (for PC) iRYS (complies with ISDP*10003:2020 as per EN ISO/IEC17065:2012 certificate number 2019003109-2) Supported protocols DICOM 3.0, TWAIN, VDDS DICOM nodes IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft* Windows* 10 Pro 64 bit - Windows* 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-A Power supply +5V ± 10%		SENSOR TECHNICAL SPECIFICATIONS	
Integrated RAM memory 4 MB (maximum 1 preservable image) Image transmission technology Wireless Wireless Operating distance Up to 2.5 m from docking station Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV. Portable: 2-10 mA and 60-70 kV. Complete recharge time 3.5 h (allows acquisition of 140* consecutive images, with a 40 s pause between two examinations) Minimum advisable recharge time 15 minutes (allows acquisition of 19* consecutive images, with a 40 s pause between two examinations) SOFTWARE Acquisition software (for PC) iCapture with dedicated filters for third party software Image management software (for PC) iRYS (complies with ISDP®10003:2020 as per EN ISO/IEC17065:2012 certificate number 2019003109-2) Supported protocols DICOM 3.0, TWAIN, VDDS DICOM nodes IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft* Windows* 10 Pro 64 bit - Windows* 11 Pro 64 bit Processor 6th generation Intel 15 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-A Power supply +5V ± 10%	Internal battery	Rechargeable lithium ion (capacity 19 mAH)	
Image transmission technology Wireless Wireless operating distance Up to 2.5 m from docking station Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV. Portable: 2-10 mA and 60-70 kV. Complete recharge time 3.5 h (allows acquisition of 140* consecutive images, with a 40 s pause between two examinations) Minimum advisable recharge time 15 minutes (allows acquisition of 19* consecutive images, with a 40 s pause between two examinations) SOFTWARE Acquisition software (for PC) iCapture with dedicated filters for third party software Image management software (for PC) iRYS (complies with ISDP®10003:2020 as per EN ISO/IEC17065:2012 certificate number 2019003109-2) Supported protocols DICOM 3.0, TWAIN, VDDS DICOM nodes IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft* Windows* 10 Pro 64 bit - Windows* 11 Pro 64 bit Processor 6th generation Intel 15 or equivalent Hard disk Intel Core i3, 10th generation (or higher) Hard disk Intel Core i3, 10th generation (or higher) 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-A Power supply +5V ± 10%	Degree of protection	IP 67 (Guaranteed against liquid or dust infiltration)	
Wireless operating distance Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV. Portable: 2-10 mA and 60-70 kV. Complete recharge time 3.5 h (allows acquisition of 140* consecutive images, with a 40 s pause between two examinations) Minimum advisable recharge time 15 minutes (allows acquisition of 19* consecutive images, with a 40 s pause between two examinations) SOFTWARE Acquisition software (for PC) Icapture with dedicated filters for third party software Image management software (for PC) Supported protocols DICOM 3.0, TWAIN, VDDS DICOM 3.0, TWAIN, VDDS DICOM nodes IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft* Windows* 10 Pro 64 bit - Windows* 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Integrated RAM memory	4 MB (maximum 1 preservable image)	
Compatibility with X-ray generators Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV. Portable: 2-10 mA and 60-70 kV. Complete recharge time 3.5 h (allows acquisition of 140* consecutive images, with a 40 s pause between two examinations) It minutes (allows acquisition of 19* consecutive images, with a 40 s pause between two examinations) SOFTWARE Acquisition software (for PC) iCapture with dedicated filters for third party software Image management software (for PC) Supported protocols DICOM 3.0, TWAIN, VDDS IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft* Windows* 10 Pro 64 bit - Windows* 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) A GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Image transmission technology	Wireless	
Complete recharge time 3.5 h (allows acquisition of 140* consecutive images, with a 40 s pause between two examinations) 15 minutes (allows acquisition of 19* consecutive images, with a 40 s pause between two examinations) SOFTWARE Acquisition software (for PC) ICapture with dedicated filters for third party software Image management software (for PC) Supported protocols DICOM 3.0, TWAIN, VDDS DICOM nodes IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft* Windows* 10 Pro 64 bit - Windows* 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card JUdeoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Wireless operating distance	Up to 2.5 m from docking station	
Minimum advisable recharge time 15 minutes (allows acquisition of 19* consecutive images, with a 40 s pause between two examinations) SOFTWARE Acquisition software (for PC) iCapture with dedicated filters for third party software Image management software (for PC) Supported protocols DICOM 3.0, TWAIN, VDDS DICOM nodes IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft® Windows® 10 Pro 64 bit - Windows® 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Compatibility with X-ray generators	Wall-mounted or cart (both AC and DC): 2-10 mA and 60-70 kV. Portable: 2-10 mA and 60-70 kV.	
Acquisition software (for PC) iCapture with dedicated filters for third party software Image management software (for PC) iRYS (complies with ISDP®10003:2020 as per EN ISO/IEC17065:2012 certificate number 2019003109-2) Supported protocols DICOM 3.0, TWAIN, VDDS DICOM nodes IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) **MINIMUM SYSTEM REQUISITES** Supported operating systems Microsoft® Windows® 10 Pro 64 bit - Windows® 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD **COMMUNICATION INTERFACES** Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Complete recharge time	3.5 h (allows acquisition of 140* consecutive images, with a 40 s pause between two examinations)	
Acquisition software (for PC) ICapture with dedicated filters for third party software Image management software (for PC) Supported protocols DICOM 3.0, TWAIN, VDDS IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft® Windows® 10 Pro 64 bit - Windows® 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Minimum advisable recharge time	15 minutes (allows acquisition of 19* consecutive images, with a 40 s pause between two examinations)	
Image management software (for PC) IRYS (complies with ISDP®10003:2020 as per EN ISO/IEC17065:2012 certificate number 2019003109-2) Supported protocols DICOM 3.0, TWAIN, VDDS IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft® Windows® 10 Pro 64 bit - Windows® 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply	SOFTWARE		
Supported protocols DICOM 3.0, TWAIN, VDDS DICOM nodes IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft® Windows® 10 Pro 64 bit - Windows® 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Acquisition software (for PC)	iCapture with dedicated filters for third party software	
Supported protocols DICOM 3.0, TWAIN, VDDS DICOM nodes IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft® Windows® 10 Pro 64 bit - Windows® 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Image management software (for PC)	iRYS (complies with ISDP®10003:2020 as per EN ISO/IEC17065:2012 certificate number 2019003109-2)	
DICOM nodes IHE compliant (Print; Storage Commitment, SR document; WorkList; MPPS; Query/Retrieve) MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft® Windows® 10 Pro 64 bit - Windows® 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Supported protocols		
MINIMUM SYSTEM REQUISITES Supported operating systems Microsoft® Windows® 10 Pro 64 bit - Windows® 11 Pro 64 bit Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	DICOM nodes		
Processor 6th generation Intel i5 or equivalent Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%		MINIMUM SYSTEM REQUISITES	
Hard disk Intel Core i3, 10th generation (or higher) RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Supported operating systems	Microsoft® Windows® 10 Pro 64 bit - Windows® 11 Pro 64 bit	
RAM 4 GB (8 GB or superior recommended) Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Processor	6th generation Intel i5 or equivalent	
Graphics card 3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support) 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply 45V ± 10%	Hard disk	Intel Core i3, 10th generation (or higher)	
Display 1920x1080 pixel 24bit RGB Full HD COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	RAM	4 GB (8 GB or superior recommended)	
COMMUNICATION INTERFACES Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Graphics card	3D VideoCard 1 GB RAM (DirectX 11 / OpenCL v1.2 or later support)	
Docking station connection port USB-C PC/laptop connection port USB-A Power supply +5V ± 10%	Display	1920x1080 pixel 24bit RGB Full HD	
PC/laptop connection port USB-A Power supply $+5V \pm 10\%$	COMMUNICATION INTERFACES		
Power supply $+5V \pm 10\%$	Docking station connection port	USB-C	
	PC/laptop connection port	USB-A	
Desire and the second s	Power supply	+5V ± 10%	
input power 2,5 W	Input power	2,5 W	

* Values susceptible to a reduction in performance due to effective battery life (the battery must only be replaced by qualified technicians)

